

high concentration (10^9 cfu/mL; Colony Forming Units/mL); both types of bacteria; PB and NB; were used in this case at the same concentration; a voltage around 1.39V for the PB and 0.18 V for NB were detected.

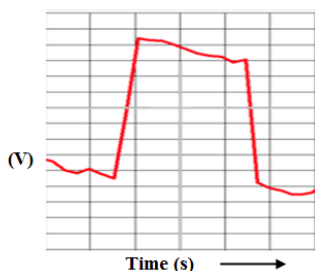


Fig. 8. The profile of fluorescent material detection after encapsulating the optical chip.

The experiment was repeated after the optical chip was encapsulated using Norland Optical Adhesives; NOA60 are clear, colorless, one part adhesives that contain no solvents. When exposed to ultraviolet light, they gel in seconds and full cure in minutes to give a tough, resilient bond. These adhesives are designed for fast, precision bonding where low strain and optical clarity are required; the following experiments have been done. A profile was recorded as a result of flowing DI water through MFC and then fluorescent material; respectively. The profile result as shown in Fig. 8 it is recording no significant difference from the previous experiment results. This means that encapsulating is significant to protect MLoC system without any influence.

V. CONCLUSIONS

Attributable to its compact design and multiplex capability, the CMOS microchip system combined with phototransistors provided high-gain and throughput analysis as tool for the detection of bacteria in medical diagnosis, food-safety inspection and bacterial pathogens DNA microarray analysis. Based on its compactness, low cost, multiplex capability, selective and sensitive method, the integrated CMOS microchip system as a detector is expected to be compatible with conventional micro-fabricated devices. This technique is allowing more rapid and high throughput analysis.

REFERENCES

- [1] J.R. Lakowicz, "Enhanced oxygen detection using porous polymeric gratings with integrated recognition elements", *Principles of Fluorescence Spectroscopy*, Kluwer Academic/ Plenum Publishers, New York, 1999.
- [2] J.R. Lakowicz, *Principles of Fluorescence Spectroscopy*, Kluwer Academic/ Plenum Publishers, New York, 1999.
- [3] Magdalena Gabig-Ciminska, Marcin Los, Anders Holmgren, Jörg Albers, Agata Czyn, Reiner Hintsche, Grzegorz Węgrzyn, and Sven-Olof Enfors, "Detection of bacterial pathogen DNA using an integrated complementary metal oxide semiconductor microchip system with capillary array electrophoresis", *Analytical Biochemistry* 324, 84–91, 2004.
- [4] Lei Yao, Mohamad Hajj Hassan, Vamsy Chodavarapu, Arghavan Shabani, Beatrice Allain, Mohammed Zourob, Rosemonde Mandeville, "CMOS Imager Microsystem for Multi-Bacteria Detection", *IEEE* 2006.
- [5] N. Nikkhou, C. Man, K. Maxwell, P. G. Gulak, "A 0.18 μ m CMOS Integrated Sensor for the Rapid Identification of Bacteria", *IEEE International Solid-state Circuit Conference*, pp. 636-617, 2008.
- [6] Turgut Sefket Aytur, "A CMOS Biosensor for Infectious Disease Detection", *Electrical Engineering and Computer Sciences, University of California at Berkeley*.
- [7] L. Gervais, M. Gela, B. Allain, M. Tolba, L. Brovko, M. Zourob, R. Mandeville, M. Griffiths, S. Evoy, "Immobilization of biotinylated bacteriophages on biosensor surfaces", *Sensors and Actuators B* 125 (2007) 615–621.
- [8] R. J. Baker: "CMOS Circuit Design, Layout and Simulation", 2nd ed., New York: Wiley-IEEE Press, 2008.
- [9] *Escherichia coli O157:H7*. CDC Division of Bacterial and Mycotic Diseases. http://www.cdc.gov/ncidod/dbmd/diseaseinfo/escherichiacoli_g.htm. Retrieved on 2007-01-25.
- [10] Abdullah Tashtoush, Adel Omar Dahmane, "Multi-Labs-On- a Chip (MLoC) For Atto-molar Cancer Markers Concentration Using VPNP Phototransistor Detection", *Manuscript submitted to be published*.
- [11] Abdullah Tashtoush, Adel Omar Dahmane, "A new generation for multibiosensors", *Manuscript submitted to be published*.
- [12] L. Yao, A. Tashtoush, E. Ghafer-Zadeh, R. Mandeville, V. Chodavarapu, "CMOS Imaging of Biological and Chemical Sensor Microarrays", Presented at the Canadian Institute for Photonics Innovation (CIPI) Annual Meeting, Quebec city, May 2009.
- [13] Vamsy P. Chodavarapu, Daniil O. Shubin, Rachel M. Bukowski, Albert H. Titus, Alexander N. Cartwright, and Frank V. Bright, "CMOS-based phase fluorometric oxygen sensor system", *IEEE Transactions On Circuits And Systems—I: Regular Papers*, Vol. 54, No. 1, January 2007.
- [14] Lei Yao, Rifat Khan, Vamsy P. Chodavarapu, Vijay S. Tripathi, and Frank V. Bright, "Sensitivity-Enhanced CMOS Phase Luminometry System Using Xerogel-Based Sensors", *IEEE Transactions On Biomedical Circuits And Systems*, PP. 1-8.